



Moving Health Forward

Florien Fife

User Manual



Important:

Read carefully before use and retain for future reference.

It is the carer/user's responsibility to ensure they are fully aware of and have understood all the safety and other instructions contained in these pages before installing or using the chair.

Contents

1. Introduction to the Florien Fife Chair	4
1.1. Why is There a Need for this Type of Chair?	4
2. Warranty Guidelines	5
2.1. Warranty and Liability	5
2.2. Use	5
2.3. When the Warranty will not Apply	5
2.4. When the Warranty Does Apply	5
2.5. Statutory Rights.....	5
2.5. Warning.....	5
3. Clinical Application	6
3.1. Intended Use	6
3.2. Who is the Florien Fife Suitable for?	6
3.3. Who is the Florien Fife not Suitable for?.....	6
4. Product Information	6
4.1. Product Identification	6
4.2. Key Features	6
4.3. Pressure Management Option	7
4.4. Accessories	7
5. Guideline for Best Practice	7
6. Instructions for Use	8
6.1. General Operation.....	8
6.2. Castors.....	9
6.2.1. Directional Lock Castors.....	9
6.3. Tilt-in-Space.....	9
6.3.1. Operation.....	9
6.4. Legrest Elevation	10
6.5. Built-in Headrest	10
6.6. Removable Arms	10
6.7. Height Adjustable Flip-Up Footrest	11
6.8. Waterfall Backrest.....	11
7. Accessories	12
7.1. Lateral Supports	12
7.2. Lap-Belt and D-Ring Fixing	12
7.3. Four Point Harness	13
7.4. Pelvic Positioner.....	14
8. Re-Use and Re-Issue	15
8.1. Modularity.....	15
8.1.1. Seat Modules	15
8.1.2. Waterfall Backrest Cushions	15
8.1.3. Arm Modules.....	15
8.1.4. Legrest Cushion	15
8.2. Disposal of the Chair	15
9. Care and Maintenance	16
9.1. Service Life	16
9.2. Periodic Checks.....	16
9.3. Cleaning	16
9.3.1. Frame Cleaning	17
9.3.2. Upholstery Cleaning.....	17
10. Technical Data	18
10.1. Manufacturing Address	18
10.2. Maximum User Weight	18
10.3. Weight and Dimensions of the Chair.....	18
10.4. Product Standards	18
10.4.1. Flammability Testing	18
10.4.2. Strength, Stability, Durability, Risk and Safety.....	19
10.4.3. Quality and Environmental	19
11. Customer Support	19

1. Introduction to the Florien Fife Chair

Thank you for purchasing a Direct Healthcare Group (DHG) Florien Fife chair.

The purpose of the Florien Fife chair is to provide a configurable modular chair that can meet a variety of user needs for those with moderate to severe seating difficulties and for those seated for lengthy periods.

Designed to easily adjust the tilt-in-space positioning without over-exertion by the carer or indeed the user, the Florien Fife integrates into many caring environments.

Meeting the needs of a higher specification product than the purely foam-based chairs the Florien Fife offers considerable support, dynamic movement and mobility.

1.1. Why is There a Need for this Type of Chair?

The ability of a seated person to function efficiently and perform activities depends on their ability to adopt the appropriate posture. All activity is posture dependent. If a person cannot move or has difficulty adjusting their posture, it may be necessary to use seating to try to provide externally what is limited internally.

The Florien Fife helps fulfil the need to maintain an individual's seated posture yet re-orientate and redistribute pressure. This is achieved by using the tilt-in-space and legrest elevation properties that are key to the functionality of the Florien Fife chairs.

2. Warranty Guidelines

2.1. Warranty and Liability

Direct Healthcare Group provides a warranty to the buyer that the goods supplied will be free from defect of workmanship, design or materials for a period of twelve (12) months from date of delivery. The Florien Fife chair frame has a ten (10) year warranty, subject to warranty guidelines 2.3 – 2.4, excluding damage to castors and upholstery. An annual maintenance service is recommended but not essential.

2.2. Use

- a) Each Direct Healthcare Group product is designed to a high specification for a particular type of use.
- b) It is important therefore that the correct product is purchased by the buyer. If the buyer intends to purchase goods for a non-approved use he must use his own skill and judgment.
- c) No employee or agent of Direct Healthcare Group is authorised to recommend non-approved uses, and the buyer should not rely on such recommendations.
- d) User instructions should be followed in all respects.

2.3. When the Warranty will not Apply:

- a) Use of incorrect cleaning products that may damage the surface material.
- b) Incorrect maintenance not approved by Direct Healthcare Group.
- c) Alterations by the buyer to the original goods.
- d) Incorrect means of transportation of the goods.
- e) Normal wear and tear.
- f) Non Approved uses:
 - Sitting on the arms of a chair.
 - Sitting on the legrest or footrest of a chair.
 - Hitting the chair against people and other objects such as doors, beds, tables, chairs, etc.
 - Spilling food, urine, excrement and other matter on the chair and not cleaning it off within a very short time of spillage (2 minutes) often causes the chair to smell and become a health hazard. Also, matter penetrates covering material, seams and foam.
 - Excessive force is often applied to the moving parts of chairs thereby breaking or bending metal and wood parts.
 - Bumping chairs up or down stairs or over obstructions with a person seated in the chair causes damage to wheels, framework and upholstery.

2.4. When the Warranty Does Apply:

Direct Healthcare Group will:

- a) Rectify the defect
- or
- b) Where in the opinion of Direct Healthcare Group, rectification is impossible, the product will be replaced.

2.5. Statutory Rights

Nothing contained in our Terms and Conditions nor in these guidelines shall affect the statutory rights of the consumer.

2.6. Warning

In this manual, warnings are indicated by symbols. The warning symbols are accompanied by a heading that indicates the severity of the danger.



WARNING

Indicates a hazardous situation that could result in serious injury or death if it is not avoided.



CAUTION

Indicates a hazardous situation that could result in minor or slight injury if it is not avoided.



IMPORTANT

Indicates a hazardous situation that could result in damage to property if it is not avoided.

3. Clinical Applications

3.1. Intended Use

The Florien Fife is intended for the following user environments:

- Care facilities such as nursing and residential care homes
- Hospital environments
- Hospice care
- Community living
- Private residences
- Single or multi-user environments

3.2. Who is the Florien Fife Suitable for?

The Florien Fife is appropriate for the following users:

- Semi-ambulant and non-ambulant users who require assistance getting in and out of the chair.
- Users requiring moderate postural support when seated.
- Users that side transfer
- Users at low to medium risk of pressure injuries (chairs fitted with Reflexion™ seat foam)
- Users at high risk or with up to a Grade II pressure injury (chairs fitted with an Intelli-Gel® seat) following a clinical assessment
- Users at very high risk or with up to a Grade IV pressure injury (chairs fitted with an Intelligent Air seat) following a clinical assessment.
- Users with mild to severe cognitive impairment.

3.3. Who is the Florien Fife not Suitable for?

The Florien Fife is not suitable for the following users:

- Fully ambulant users unless fully supervised by a healthcare professional in a treatment setting and following a clinical assessment
- Users with complex postures requiring significant support

4. Product Information

4.1. Product Identification

Each chair has a unique number to enable swift identification.

This number can be found on the underside of the legrest module of the chair.

4.2. Key Features

The Florien Fife chair incorporates a range of features to enable suitable occupants to achieve an appropriate seated position.

- Manual Tilt-in-Space action
- Manual legrest elevation
- 25° negative legrest angle to accommodate contractures at the knee or to aid standing transfers
- Ramped Seat Module
- Removable arms for easier hoist access and side transfers
- Multi-Positioning, integral headrest
- Waterfall Backrest
- Height Adjustable Flip-Up Footrest
- Fixing Plates for Pelvic Positioners
- Ergonomically positioned push handle

Sales Order No.	
Date of Manufacture.....	Direct Healthcare Group Ltd, Withey Court, Western Industrial Estate, Caerphilly, UK, CF83 1BF
Client's Name.....	Tel: +44 (0)800 043 0881
Product	
Meets B.S. 5852 for cigarette and match, also crib 5 over CMHR foam. Meets 'The Furniture & Furnishing (Fire) (Safety) Amendment Regulations 1993'	

4.3. Pressure Management Option

Pressure management is critical for those who are seated for long periods. The Florien Fife has pressure relieving foams on all contact surface areas of the chair and further options are available for the seat module in accordance with the occupant's needs.

If you are unsure about the suitability of your pressure care, please seek advice and input from a qualified Occupational Therapist, Tissue Viability Nurse, healthcare professional and/or Direct Healthcare Group representative/retailer before purchasing.

4.4. Accessories

A range of optional accessories are available for use with the Florien Fife chair. Please contact Direct Healthcare Group Customer Services Team on Freephone 0800 043 0881 or your local retailer for current pricing and availability.

NG551	Florien Fife Infill Arm Blocks 400mm (Pair)	DU701	Easicare Medium 4 Point Lap-Belt with Fixings
NG552	Florien Fife Infill Arm Blocks 450mm (Pair)	DU703	Easicare Medium 2 Point Lap-Belt with Fixings
NG553	Florien Fife Infill Arm Blocks 500mm (Pair)	DU704	Easicare Large 2 Point Lap-Belt with Fixings
NG554	Florien Fife Lateral Supports - Short Metalwork, Small Pad (Pair)	DU705	Easicare Large 4 Point Lap-Belt with Fixings
NG555	Florien Fife Lateral Supports - Short Metalwork, Large Pad (Pair)	UL706	D-Ring Straps (Long)
NG556	Florien Fife Lateral Supports - Long Metalwork, Small Pad (Pair)	NG558	Bottom Waterfall Cushion 400mm Seat Width
NG557	Florien Fife Lateral Supports - Long Metalwork, Large Pad (Pair)	NG559	Bottom Waterfall Cushion 450mm Seat Width
NG402	Florien Fife Seat Infill Block	NG560	Bottom Waterfall Cushion 500mm Seat Width
NG403	Florien Universal Headrest in Dartex	NG561	Top Waterfall Cushion
NG586	Florien Flip-Up Footrest	KB309	Laminated Tray with Straps
		KB313	Universal Mobile Tray



CAUTION

Only use accessories recommended by Direct Healthcare Group with the Florien Fife chair.

5. Guidelines for Best Practice

To ensure good practice when considering purchasing a Florien Fife chair and effective use post purchase we advise that the following guidelines are considered:

- Seek advice and input from a qualified Occupational Therapist, healthcare professional and/or Direct Healthcare Group representative/retailer at the initial prescription of the chair.
- Consideration should be given to matching the basic dimensions of the chair to the body size of the occupant to ensure good posture, support, comfort and safety. Any pressure care, moving and handling, incontinence or infection control issues should be considered and appropriate advice taken from qualified healthcare professionals.
- Environmental factors should also be considered and assessed and any potential risks or hazards should be identified and taken into consideration to ensure user safety.
- When any chair is specified we recommend that a risk assessment is conducted to ensure it will be safe and appropriate for the user(s) of the chair and for all who may find themselves in the vicinity of the chair. Regular reassessment as to the suitability of the product for the user is important.
- All care-givers that will be supervising the user(s) should be trained in operating the chair to ensure correct positioning of the occupant is achieved.

6. Instructions for Use

The purpose of these user instructions is to ensure the safe operation, adjustment and maintenance of your Florien Fife chair.

The chair is ready for use once fully installed in the correct position and all carers/users have read and understood the operating instructions.

Safety advisories are included within these user instructions and it is the operator's responsibility to ensure these are read and fully understood. If you have any questions or concerns, please contact your Direct Healthcare Group representative, retailer or the Direct Healthcare Group Customer Care Team on **Freephone 0800 043 0881**.

Please retain these instructions for future reference.

6.1. General Operation

Products must **never** be modified or altered after purchase other than by Direct Healthcare Group authorised personnel.

It is important that Florien Fife chairs are used appropriately, if there is any doubt as to the suitability of the product for the user, professional advice should be sought from a qualified healthcare professional such as an Occupational Therapist, Physiotherapist, Tissue Viability Nurse or a moving and handling specialist.

If you wish to discuss safety issues in more detail please telephone our Customer Care Team on **Freephone 0800 043 0881**.



CAUTION

When the chair is in use, always ensure the user is checked regularly for safety and is not left unattended for long periods of time.



WARNING

Do not push the chair up or down steps or a steep incline as this could result in loss of control.



WARNING

The Florien Fife is not suitable for use by children. Any children present in the vicinity of the chair must be supervised at all times.



WARNING

Ensure there is nothing present to obstruct the free movement of the chair before attempting to use the chair.



CAUTION

Do not sit on the arms of the chair at any time.

6.2. Castors

The Florien Fife is fitted as standard with four 100mm/4" castors with two swivel castors at the front and two locking castors at the rear that will not roll or swivel when the brakes are activated.

To **apply** the brakes on the braked castors, press down on the **red** front edge of the ridged pad on each castor (Fig 1).

To **unlock** the brakes, gently push down with your foot, the raised top of the ridged pad until it is level with the rest of the castor housing (Fig 2). The castor should roll freely.



Locked



WARNING

Ensure the castor brakes are applied at all times when the occupant is left unattended in the chair.



WARNING

Ensure castor brakes are applied when the occupant is being transferred in or out of the chair to avoid any unexpected movement of the chair.



Unlocked



WARNING

Ensure all four wheels are in contact with the floor surface before leaving the patient unattended.



WARNING

Ensure the chair is on an even surface before leaving the patient unattended.



CAUTION

Ensure there is nothing present to obstruct the free movement of the chair before releasing the brake and attempting to move the chair.



CAUTION

Always check that the castors are unlocked before moving the chair.

6.2.1. Directional Lock Castors *(optional accessory)*

The Florian Fife chairs can be fitted with a directional lock castor as an optional accessory. This allows one castor to be locked in the 'straight-ahead' direction.

The back right wheel is a directional locking castor (green) that can be locked in the straight ahead position making it easier to push the chair in a straight line.

- Press down on the green front edge of the ridged pad. Then push the chair forwards to activate the directional lock.

It will "click" when in the straight ahead position.

- To deactivate the directional castor, press down on the top edge of the green ridged pad until it is level with the top edge of the rest of the wheel.
- Ensure the directional lock castor is deactivated before manoeuvring the chair in tight spaces.
- The remaining three castors will be fully locking castors with a red tab that will not roll or swivel when the brake is activated.



6.3. Tilt-in-Space

What is Tilt-in-Space?

Tilt-in-space is a pivoting system that provides a reclined, resting position whilst maintaining posture and pelvic stability.

The main purpose of tilt-in-space positioning is to decrease the pressure in the buttocks area and to provide muscle relaxation in the lower part of the back.

Tilting the chair re-distributes the occupant's weight over a larger contact surface area, making a simple yet effective way to combat the build-up of pressure in the buttocks area.

6.3.1. Operation

It is recommended that the tilt-in-space angle is changed at regular intervals to reduce the risk of the occupant developing pressure sores.

Locate the lever on the right hand side of the push handle at the rear of the chair and squeeze towards the push handle to release the tilt lock.

Apply firm downward pressure with both hands on the push handle to tilt the chair backwards, or lift the push handle upwards to raise the chair.

- At any point during the upward or downward tilt motion the lever can be released and the chair will lock in the selected position.
- It is always advisable to adjust the positioning of the legrest once the tilt-in-space positioning has been chosen, to ensure a correct and comfortable posture.



CAUTION

It is recommended to use a lap-belt or pelvic positioner (optional accessories) with users with poor postural sitting ability.



WARNING

Never leave a user with poor postural sitting ability in a fully upright position without supervision as they may tip forwards out of the chair.



WARNING

Ensure the occupant's hands are clear from the back of the chair whilst the chair is being tilted, to avoid any risk of pinching within the tilt mechanism.



WARNING

Ensure there is nothing present to obstruct the free movement of the chair (e.g. children, pets or solid objects) before operating the tilt-in-space.

6.4. Legrest Elevation

Locate the legrest release lever at the bottom of the right hand arm, towards the front castor (when viewed from the rear)

The legrest can be elevated or retracted by pulling the lever with the left hand whilst moving the legrest with the right hand and then releasing the lever to lock the legrest in position. This enables the carer to retain some eye contact with the occupant.

A negative legrest angle can be achieved with the legrest to accommodate occupants with fixed contractures as well as to aid exiting the chair.

Lower the legrest before returning the chair to its fully upright position to allow the user to stand up from the chair with ease.



IMPORTANT

Do not sit on the legrest. The legrest is not designed to support the weight of an adult



WARNING

When retracting the legrest, keep hands clear of the seat cushion, to avoid any risk of pinching fingers.



WARNING

When retracting the legrest, ensure the occupant's legs are in the middle of the legrest to avoid the risk of trapping the occupant's legs or feet between the legrest and chair frame.



WARNING

Ensure there is nothing present to obstruct the free movement of the chair (e.g. children, pets or solid objects) before operating the legrest elevation.

6.5. Built-in Headrest

The built-in headrest is an integral part of the back of the Florian Fife chair. The pivot point is located approximately 30cm (12 inches) from the top of the chair.

To adjust the headrest:

Stand behind the chair and place one hand on the push handle. Use the other hand to push firmly on the top of the backrest forward until the headrest is in the desired position.

The friction lock will ensure this position is maintained and will not move when the chair is occupied.



IMPORTANT

When lowering the legrest, or returning the chair from a tilted to upright position, it is advisable to adjust the (optional) footrest to the shortest position or remove it entirely to prevent damage to the footrest or floor. If left extended, it will fall on the floor when the chair is tilted forward and could be damaged.

6.6. Removable Arms

This unique feature of the Florian chairs enables either side transfer to be effected or facilitates easier hoist access.

To remove the arms:

- If the chair is tilted, first return the chair to an upright position.
- If lateral supports are being used these should be removed from the chair.
- Stand at the side of the chair and hold the arm at the rear corner and the front where the arm meets the seat. Lift the arm up gently and away from the chair.

To replace the arms:

- Pick up the removed arm module, holding it at the rear corner and the front where the arm would meet the seat.
- Stand at the side of the chair and position the arm so it rests above the seat cushion.
- Guide the metal plate on the inside of the arm onto the metal bracket next to the seat cushion and push down firmly.
- The back of the arm should line up closely to the backrest and the front of the arm should meet the top of the seat.



WARNING
Always check the arm is securely in place before using the chair.

WARNING
Do not remove arm if occupant has poor sitting balance.

WARNING
Do not sit on the arms of the chair at any time.

WARNING
Always apply the brakes to the chair attempting a side transfer into or out of the chair.

WARNING
Use a transfer board or slide sheet when transferring a patient sideways, to prevent risk of injury to the occupant.


WARNING
Extreme care should be taken when removing the arms to ensure that the occupant of the chair does not fall sideways or out of the chair.

WARNING
Check the arm is securely in place by attempting to pull the arm from side to side, before leaving the occupant unattended.

6.7. Height Adjustable Flip-Up Footrest

The height adjustable footrest provides added support and positioning for the feet and is highly recommended to avoid foot-drop and other similar conditions.

The footrest can be raised to lie against the legrest when entering or exiting the chair and folds down when in use. When lowered, the footrest sits at 90° to the legrest.

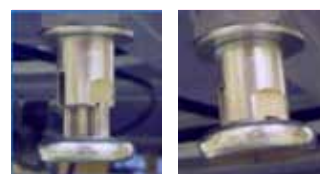

Unlocked

Locked

WARNING
The carer should keep hands clear of the footrest hinge whilst operating the flip-up footrest to avoid risk of pinching fingers.

The footrest on the Florian Fife chair is height adjustable:

- Raise the legrest to the desired angle (refer to section 6.4)
- The complete footrest height should then be adjusted by releasing two spring-loaded “snaps” which engage in holes in the metalwork of the legrest
- The “snaps” are located behind the legrest framework. Reach around the legrest and pull out both pins and turn them to 90° to enable the footrest to be positioned.
- Slide the footrest up or down as required and turn the snaps back through 90° allowing the snaps to click into the required hole.
- Only when the snaps audibly click into place will the footrest be secure.

WARNING
Ensure the snaps are fully locked and the footrest is secure before leaving the occupier unattended.

6.8 Waterfall Backrest

The Florian Fife has a Waterfall Backrest. This is comprised of four waterfall cushions – the top and bottom cushions are held in place with Velcro while the middle two cushions are stitched onto the back module.

Ensure all cushions are fitted in their designated position to ensure the comfort and correct positioning of the chair’s occupant. The required size for the lower waterfall cushion is determined by the chosen seat width of the chair.

7. Accessories

A range of optional accessories are available for use with the Florian Fife chair. Contact the Direct Healthcare Group Customer Care Team on Freephone 0800 043 0881 or your local retailer for current pricing and availability.

If you are unsure about the suitability of any of these accessories for your Florian Fife chair, please seek advice and input from a qualified Occupational Therapist, healthcare professional and/or Direct Healthcare Group representative/retailer before purchasing.

7.1. Lateral Supports

Lateral supports help to maintain an individual's posture and encourage an appropriate midline position.

Lateral Supports are generally used as a pair with one fitted to either side of the Florian Fife chair. They adjust independently but operate in the same way.

The lateral supports attach to the chair through the lateral support bar at the back of the chair.

To attach or detach the lateral supports, simply unscrew the "triangular" handle and slide each support into or from the bracket at the back of the chair.

- The two lateral supports can be moved horizontally (wider or narrower) or rotated vertically (up and down) to support the occupant of the chair.
- When appropriate positioning has been found then the "triangular" handles should be tightened to provide stable and secure support.



IMPORTANT

Both lateral supports can be completely removed when required or rotated to the back of the chair. This is essential during the removal of the arm modules.



7.2. Lap-Belt and D-Ring Fixing

The Lap-Belt helps stabilise the pelvis and position the occupant in the back of the chair to achieve a good sitting posture and reduce the risk of tissue damage through the effects of shear which can occur if the occupant has an unstable posture.

When using a Lap-Belt a level of supervision appropriate to the occupants abilities must be applied at all times.

All Lap-Belts need to be correctly adjusted to adequately support the occupant without restricting breathing or causing discomfort.

It is essential the Lap-Belt does not fit loosely around the occupant and is not allowed to work loose over time as this will allow the pelvis to tilt backwards, encouraging the occupant to slide down and forward in the chair, particularly if in an upright position.

Ideally the D-Ring fixings for the Lap-Belt and the Lap-Belt itself will be fitted at time of manufacture however; it can be fitted retrospectively by a trained representative (refer to D-Ring fixing).

To use the Lap-Belt effectively, undo the buckle joining the two halves of the strap by depressing the button on the central console and place the straps over the arms or to the side of the seat before transferring the occupant into the chair.

When the occupant is seated correctly, bring the two sides of the buckle together and fasten.

To adjust the Lap-Belt, pull on the plastic loop to give firm control but take care not to restrict the occupant's movement. The Lap-Belt is designed to pull back over the hips at an angle between 45° and 60°.

This angle helps to maintain a vertical pelvis by simultaneously positioning the hip joint down and back.



D-Ring Fixing

The chair may come pre-fitted with D-Ring straps if ordered at the time of manufacture. If so, these will normally be visible near the interface between the seat module and the back cushion. In this case, the Lap-Belt can be fixed to the D-Rings by simply snapping the spring clip on the end of the Lap-Belt onto the visible D-Ring.

If the chair is not already fitted with D-Rings, these should be attached to a rigid part of the chair's metal framework on either side of the seat module in order they can feed through between the seat and arm modules.



WARNING

If the Lap-Belt is too loose there is a risk of the occupant sliding underneath or into an inappropriate position. The Lap-Belt should be checked for correct tightness, regularly. Care should be taken not to over tighten the Lap-Belt in order to reduce the risk of harm to the occupant.



WARNING

The webbing and plastic fittings should be checked at least weekly for any signs of damage. If damaged, the Lap-Belt should not be used.



WARNING

The occupant is at risk if the Lap-Belt is not properly specified and adjusted to their particular requirements.



WARNING

Thrusts, spasms and strong movements, for example, as well as partial loosening of the Lap-Belt could cause injury to the occupant.

7.3. Four Point Harness

The Four Point Harness is a useful positioning aid to prevent the occupant of the chair from sliding into an uncomfortable position.

To fit the Four Point Harness:

- Locate the metal bar at the rear of the chair, behind the seat module
- Loop each of the upper, wider straps of the Four Point Harness around this bar on either side.
- Thread the straps back through the black plastic sliders located on the straps, to secure their position.
- Use the sliders to adjust the straps to a suitable length for the occupant of the chair.
- Remove the left armrest and locate the fixing plates on the side of the seat module, under the armrest.
- Take the narrower anchor strap on the left side of the harness and thread it through the desired hole of the fixing plate, under and up. (Note: Choosing a hole nearer to the front of the chair will provide more support across the occupant's leg)
- After choosing the desired position, thread the strap back through the black plastic slider located on the strap to secure its position.
- Replace the left arm module on the chair.
- Repeat the above for the narrow anchor strap on the right side of the chair.



WARNING

Do not remove both armrests at the same time if the chair is occupied as this could affect the stability of the occupant.

7.4. Pelvic Positioner

The Pelvic Positioner is used to help position occupants securely in the back of the chair for those with low muscle tone or control in their pelvis.



Fitting the Pelvic Positioner to the chair

Ensure the chair is unoccupied before fitting the Pelvic Positioner.



Place the Pelvic Positioner in the seat of the chair with the buckles pointing towards the chair front and the clips on the buckles facing down.



Feed the lengths of the straps through the D-rings on either side of the seat module.



Place the ends of the straps over the arms of the chair ready for the occupant to transfer to the chair.

Sit the occupant into the chair with their pelvis firmly back in the seat and their buttocks on the back edge of the Pelvic Positioner.



Bring the straps over the occupant's thigh and through the buckles on each end of the Pelvic Positioner, located between the occupant's legs.



Pull the straps tight and fasten down the clips on the buckles. The fit should be snug – not too tight and not too loose.



CAUTION

Take care when adjusting positions to avoid trapping or pinching of body parts.



WARNING

Only a trained individual or a responsible person should adjust the product.



WARNING

The occupant should be regularly checked and the Pelvic Positioner adjusted to ensure optimum positioning and safety.



WARNING

Due to the risk of cross infection, this product should not be used by more than one person.

8. Re-Use and Re-Issue

While the Florien Fife chair has been tailored specifically for the planned occupant's needs at the time of manufacture, with some alterations and adjustments, the chair can be re-issued and re-used in a multi-user healthcare environment.

Please seek advice from a qualified Occupational Therapist, healthcare professional and/or Direct Healthcare Group representative/retailer before using the Florien Fife chair with another user for whom the chair was not originally specified.



WARNING

Consideration to cross infection risks must be given when reusing or reissuing chairs.



CAUTION

If using the Florien Fife chair in a multi-user environment conducting an in situ risk assessment is recommended.

8.1. Modularity

The Florien Fife chair has a durable frame with modular arm, seat and legrest components, along with a backrest comprised of three waterfall cushions. These components can be purchased separately as required, whether to replace a worn module or cushion, or to re-issue to another user.

Contact the Direct Healthcare Group Customer Care Team on **Freephone 0800 043 0881** or your local retailer for current pricing and availability.

8.1.1. Seat Modules

The Florien Fife seat module is one standard size across all Florien Fife chairs.

The seat modules are also available with three levels of pressure relief:

- Reflexion™ foam seat cushion (for those at low to medium risk of pressure injuries)
- Intelli-Gel® seat cushion (for those at high risk or with up to a Grade II pressure injury).
- Dyna-Tek® Intelligent Air seat cushion (for those at very high risk or up to a grade IV pressure injury).

A visit from a Direct Healthcare Group trained engineer will be required to fit the replacement seat module.

8.1.2. Waterfall Backrest Cushions

Replacement Waterfall Backrest cushions can be purchased for the Florien Fife chair, please contact Direct Healthcare Group Customer Care Team on **Freephone 0800 043 0881** for further information or your local retailer.

8.1.3. Arm Modules

Replacement arm modules can be purchased for the Florien Fife chair, please contact Direct Healthcare Group Customer Care Team on **Freephone 0800 043 0881** or your local retailer for further information. Arm modules can be purchased as a pair or separately as required.

The specification of the arm modules required for your chair will depend on the seat width required for the chair. Please ensure the required seat width is stated when placing an order for replacement arm modules to ensure your order is not delayed.

8.1.4. Legrest Modules

A replacement legrest cushion can be purchased for the Florien Fife chair. Please contact Direct Healthcare Group Customer Care Team on **Freephone 0800 043 0881** or your local retailer for further information.

8.2. Disposal of the chair

The Florien Fife chair consists of mostly metal, plastic, wood, foam and fabric components. Disposal of each individual material must be carried out in with the environmental and disposal regulations in the relevant country, and may only take place after the chair has been dismantled fully.



9. Care and Maintenance

Every time the chair is used, check for signs of damage or excessive wear and tear. If the chair displays signs of excessive wear and tear take out of service immediately and contact Direct Healthcare Group

Customer Care Team on **Freephone 0800 043 0881** or your local retailer for advice about repair and refurbishment.



WARNING

Failure to repair damage or wear and tear could put the occupant at risk of injury.

9.1. Service Life

The service life of the chair in normal daily use is 10 years. The framework, excluding castors and consumables, is warranted for 10 years. Upholstery and other consumables which are warranted for 12 months, such as castors, may need to be replaced within this time frame.

It is recommended that the chair is inspected by a trained service technician every year, to ensure safe operation of the product (refer to 2. Warranty Guidelines).



WARNING

If the chair develops a fault, STOP using the chair, and contact Direct Healthcare Group Customer Care Team on **Freephone 0800 043 0881** or your local retailer for further advice.

9.2. Periodic Checks

The chair should be checked every time it is used for signs of damage or excessive wear and tear to ensure safe and reliable operation.

Monthly checks should include, but are not limited to:

- Any damage to the cables or adjustment levers.
- Any loose or detached parts.
- Check castors for damage and a build-up of fluff and dirt particles.
- Any damage to the fabric of the chair including any soiling of the fabrics.

If any damage is present, STOP using the chair, and contact Direct Healthcare Group Customer Care Team on **Freephone 0800 043 0881** or your local retailer for further advice on repair and refurbishment.

9.3. Cleaning

The chair should be kept clean to preserve the life and appearance of the chair.

Regular cleaning is essential to minimise risk of cross infection between users and carers particularly in a multi-user healthcare environment.



WARNING

Check the chair for correct functioning after cleaning.



WARNING

Regular cleaning is essential to minimise the risk of infection transmission between users and carers.



IMPORTANT

To reduce the risk of infection transmission to the carer, always use protective gloves when decontaminating and cleaning the chair.

9.3.1. Frame Cleaning

The metal framework of the chair can be cleaned with a mild detergent and a soft cloth.

- ! **IMPORTANT**
Cleaning with scouring pads is not recommended.

9.3.2. Upholstery Cleaning

- ! **IMPORTANT**
Check the type of upholstery before cleaning to ensure correct agents are used.

Cadet, Venture, Berkshire and Brookland Vinyl Cleaning Instructions (External surfaces)

These vinyls have high scratch resistance and a colour solid to the base cloth.

Anti-Microbial and Anti-Fungal Protection. Tested to AATCC147.

- Clean and care for the fabric on a regular basis and it will maintain its condition and appearance. Most stains can be removed by wiping clean.
- The new generation of microfibre cleaning cloths are extremely effective with or without soap for general care and maintenance.
- Wipe clean regularly with a damp cloth to remove dust particles and light soiling.
- Remove spillages promptly (within 15 minutes) with an absorbent dry cloth.
- For heavier soiling, use a soft brush with care to avoid abrasive damage to surface and tepid soapy water (non-alkaline). Rinse clean with clear water. Dry with an absorbent cloth.
- Bodily fluids should be removed promptly (within 15 minutes) with cold water and then cleaned as above.
- Extreme soiling/infection control use a 5% sodium hypochlorite (bleach) solution.
- Do not machine wash or dry clean.
- Do not use polish or solvents.

Enduratex® Vinyl Cleaning Instructions (External Surfaces)

Enduratex® contact materials are protected by Produratec-C® lacquer coating and are resistant to every day wear and contact with mild acids, alkali, drinks, household stains.

- Use warm soapy water and/or Haz-tab or Clor-clean solution and a household cloth.
- Rub evenly in the direction of the grain of the material.
- Rinse with clean water afterwards.
- Can also be steam cleaned.

DO NOT USE bleaches, solvents, abrasives, wax polishes or aerosol sprays.

Dartex Cleaning Instructions (User Contact Surfaces)

General Guidance

- Attention must be paid to the properties of any other materials, which may be combined with Dartex Coatings fabrics in the final article (e.g. dimensional stability, colour fastness, washing instructions).
- Some surface wrinkling may result from cleaning procedures. This has no adverse effect on the fabric's properties.
- Abrasive cleaning agents should not be used.

Washing and Disinfection

- Superficial dirt on the coating may be removed by wiping with a soft cloth moistened with water containing a neutral detergent. More persistent contamination may be treated by wiping with alcohols or turpentine substitute, followed by hot water and detergent.
- Cleaning and disinfection in situ may be carried out on the coating with hand hot water and a neutral detergent or with a sodium hypochlorite solution (0.1% or 1000 parts per million available chlorine).
- Proprietary disinfectants may be used provided manufacturer's instructions are followed.
- All cleaning agents, and disinfectants, must be thoroughly rinsed off and the item dried before storage. Failure to do this may result in the accumulation of reagent that could damage the polyurethane coating, react with the chair frame, or negate the biocompatibility results of the Dartex® fabric.

Drying

- It is essential that articles be thoroughly dried after all cleaning procedures and before storage.

Storage

- Store in a cool, dry area. Avoid excessive pressure and contact with non-colourfast materials.

10. Technical Data

10.1. Manufacturing Address

Direct Healthcare Group
 Withey Court, Western Industrial Estate, Caerphilly, UK, CF83 1BF

Telephone: +44 (0) 800 043 0881

Email: info@directhealthcaregroup.com

10.2. Maximum User Weight

Maximum user weight limit **180kg (353lbs) or 28 stone**

Please adhere to the user weight limit for the Florian Fife chair and note your warranty will be void and user safety may be compromised should the weight limit be exceeded.

10.3. Weight and Dimensions of the Chair

Item	Weight (kg)	Dimensions (mm)
Florien Fife	47	880 x 700 x 1330
Florien Fife + Box + Pallet	64	1000 x 800 x 1450
Cardboard Box	7	1000 x 800 x 1300
Pallet	10	1000 x 800 x 150

10.4. Product Standards

MHRA Registration CA000105

10.4.1. Flammability Testing

- BS 7176:2007+A1:2011 (Specification for resistance to ignition of upholstered furniture for non-domestic seating by testing composites).
- BS EN 1021-1:2014 (Furniture. Assessment of the ignitability of upholstered furniture. Ignition source smouldering cigarette).
- BS EN 1021-2:2014 (Furniture. Assessment of the ignitability of upholstered furniture. Ignition source match flame equivalent).
- BS 5852:2006 (Methods of test for assessment of the ignitability of upholstered seating by smouldering and flaming ignition sources).

10.4.2. Strength, Stability, Durability, Risk and Safety

- BS EN 1022:2005 (Domestic furniture. Seating. Determination of stability).
- BS EN 16139:2013 (Furniture. Strength, durability and safety. Requirements for non-domestic seating).
- BS EN ISO 14971:2012 (Medical devices. Application of risk management to medical devices).

10.4.3. Quality and Environmental



11. Customer Support

Should you have any concerns or are experiencing any problems regarding the set up or maintenance of your Florien Fife chair please contact our Customer Care Team on **Freephone 0800 043 0881**.



Moving Health Forward

**PRESSURE ULCER PREVENTION
SAFE MOVING & HANDLING
SPECIALIST THERAPIES
BATHROOM SAFETY
RENTAL & SERVICE SOLUTIONS**



Direct Healthcare Group Ltd
Withey Court, Western Industrial Estate
Caerphilly, United Kingdom
CF83 1BF
T: +44 (0) 800 043 0881
F: +44 (0) 845 459 9832
E: info@directhealthcaregroup.com



**EU Authorised Representative, Importer
and Distributor:**

Direct Healthcare Group Sverige AB,
Torshamnsgatan 35, SE-164 40, Kista
Sweden
T: +46 (0) 8 557 200

Australian Sponsor:

Direct Healthcare Group Pty Ltd.,
68 Howe Street, Osborne Park,
Western Australia 6017
T: +61 (0) 423 852 810



LIT-00034 Issue 2
Date: February 2022

DIRECTHEALTHCAREGROUP.COM